

Fig. 1

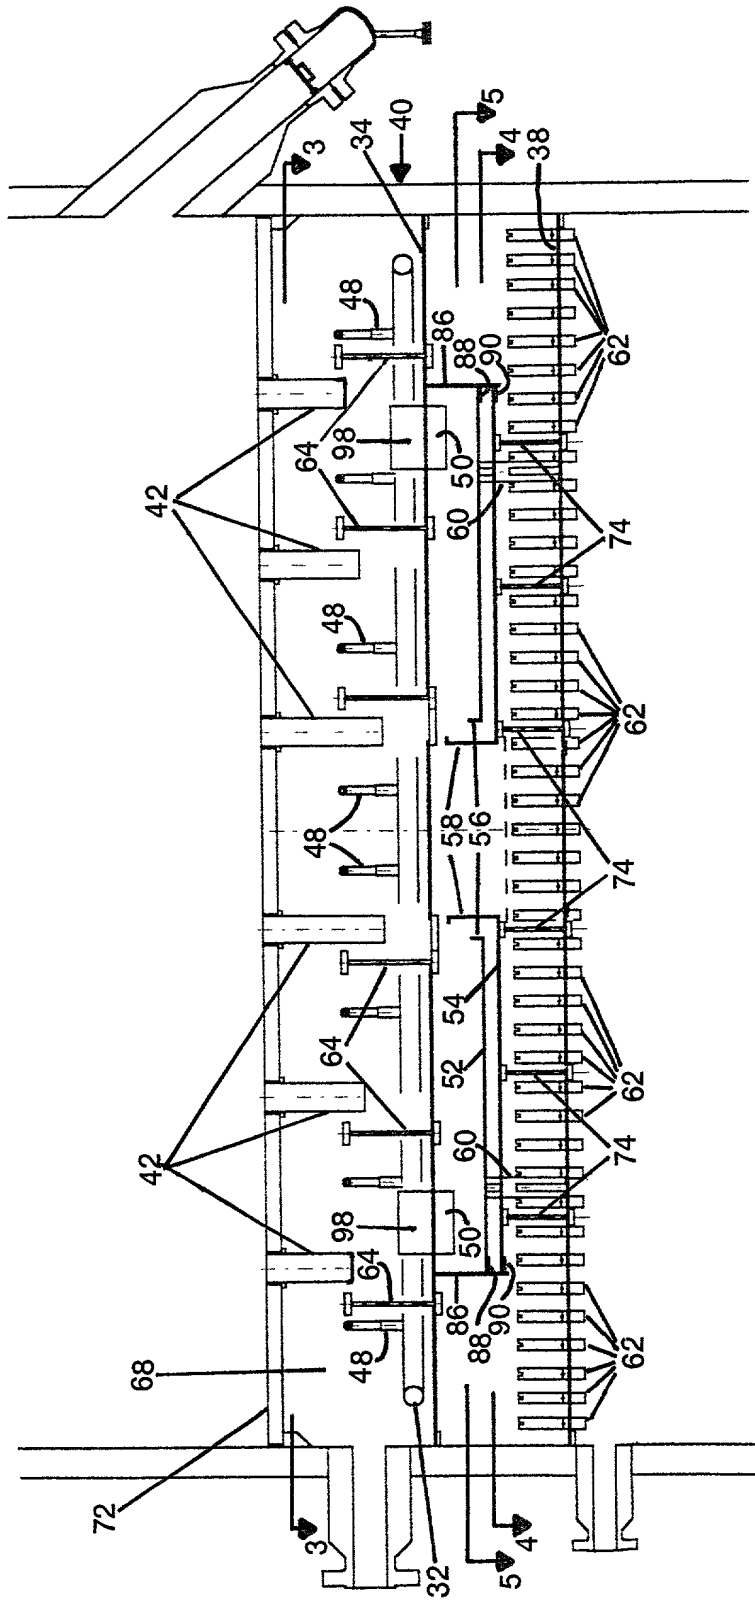


Fig 2

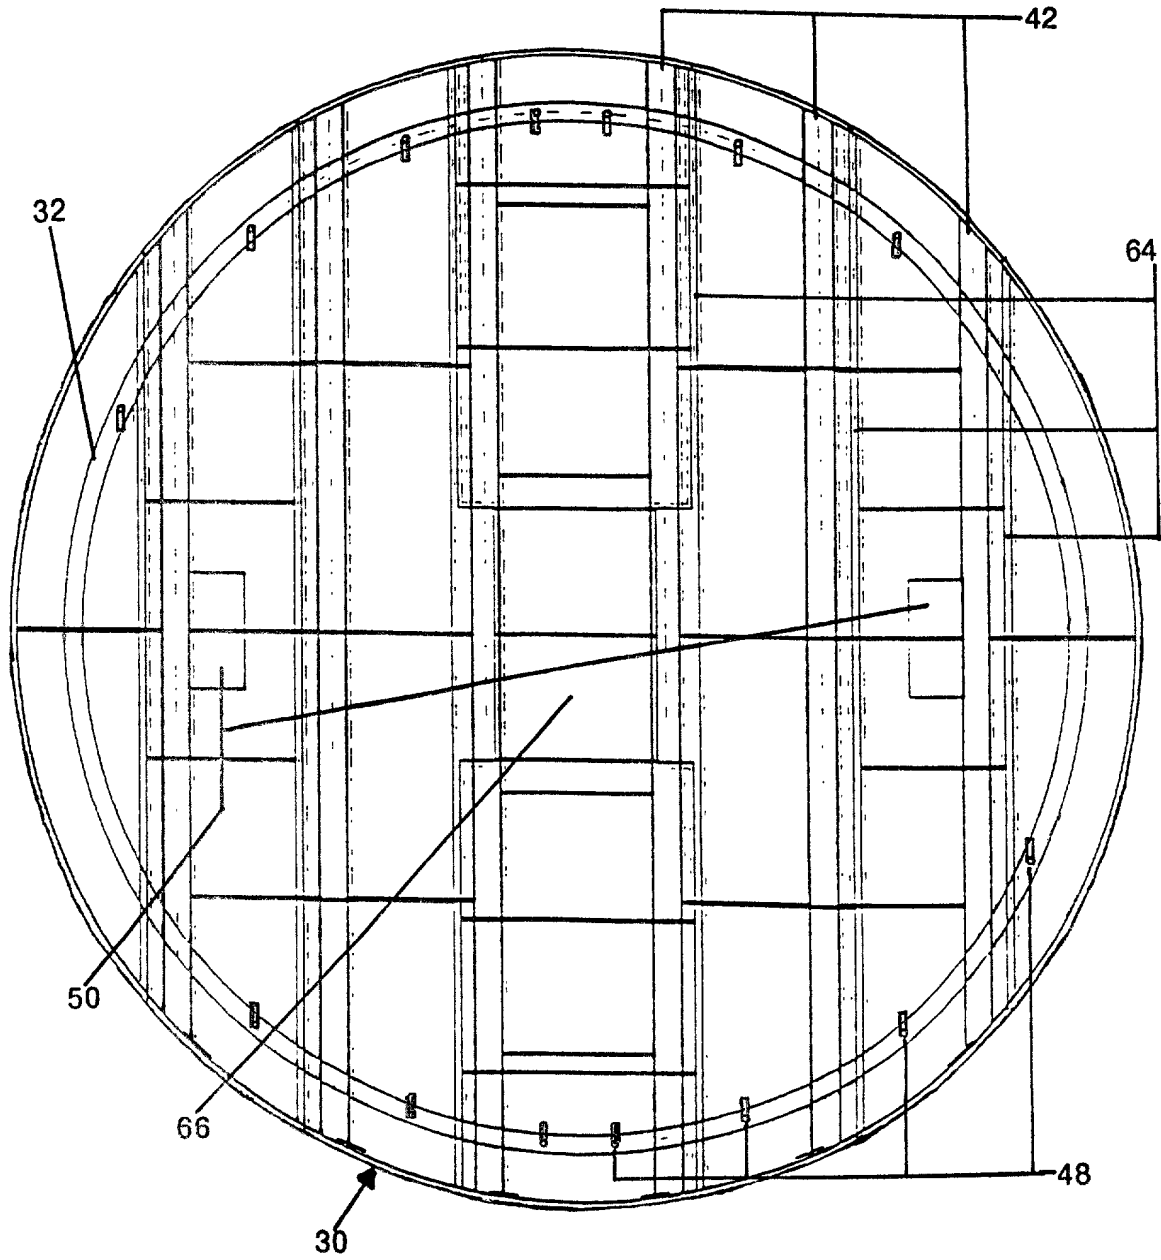


Fig 3

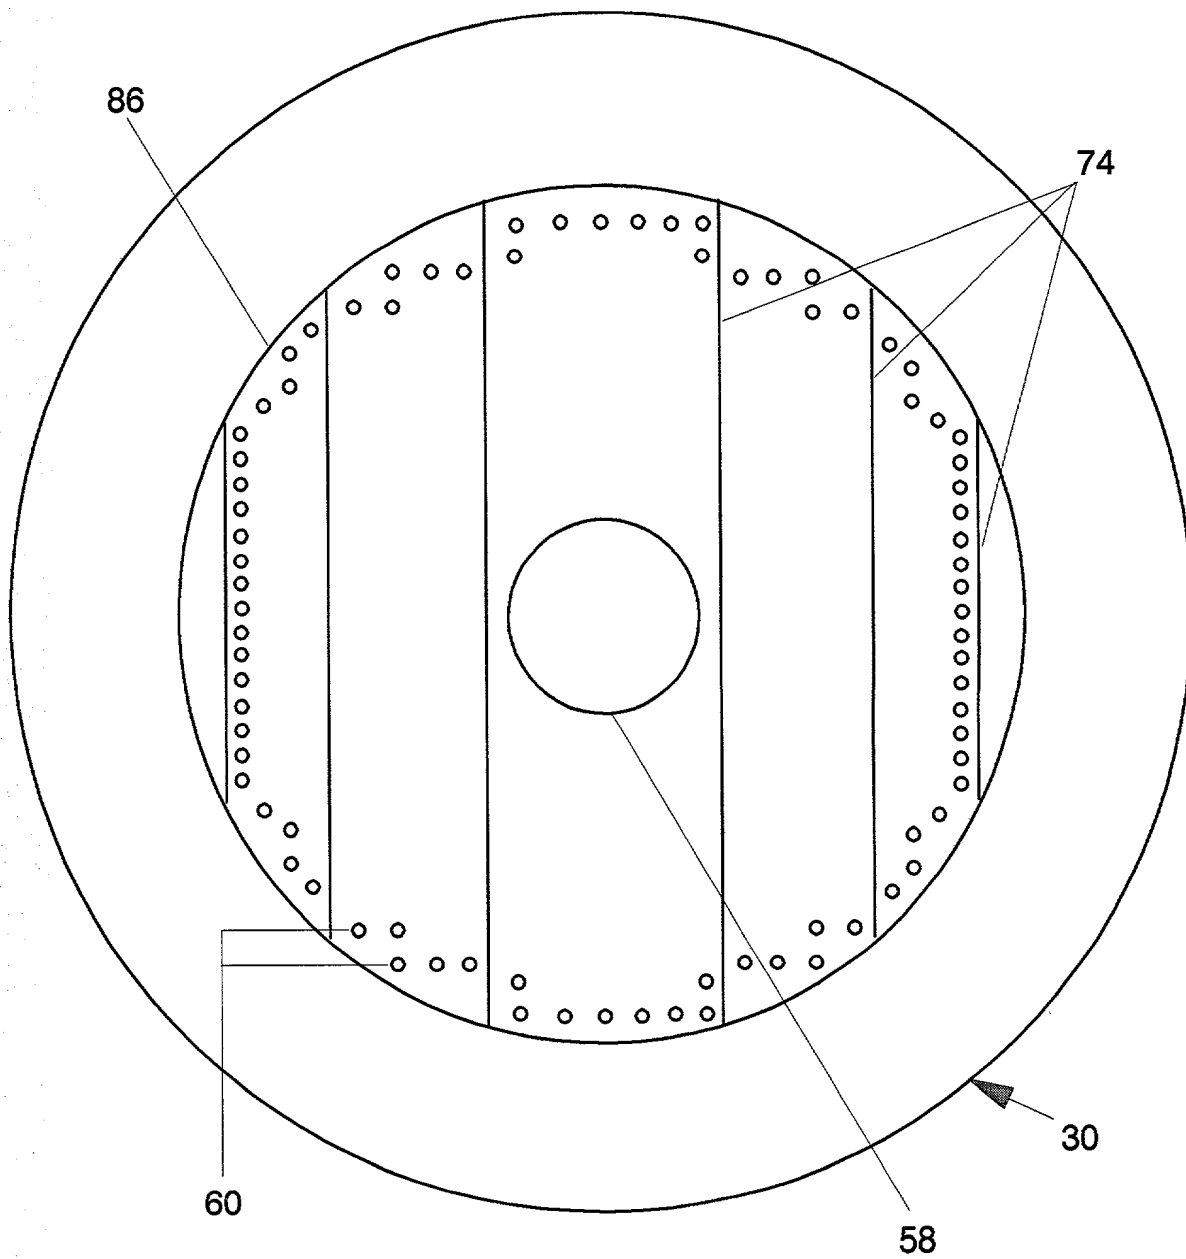


Fig. 4

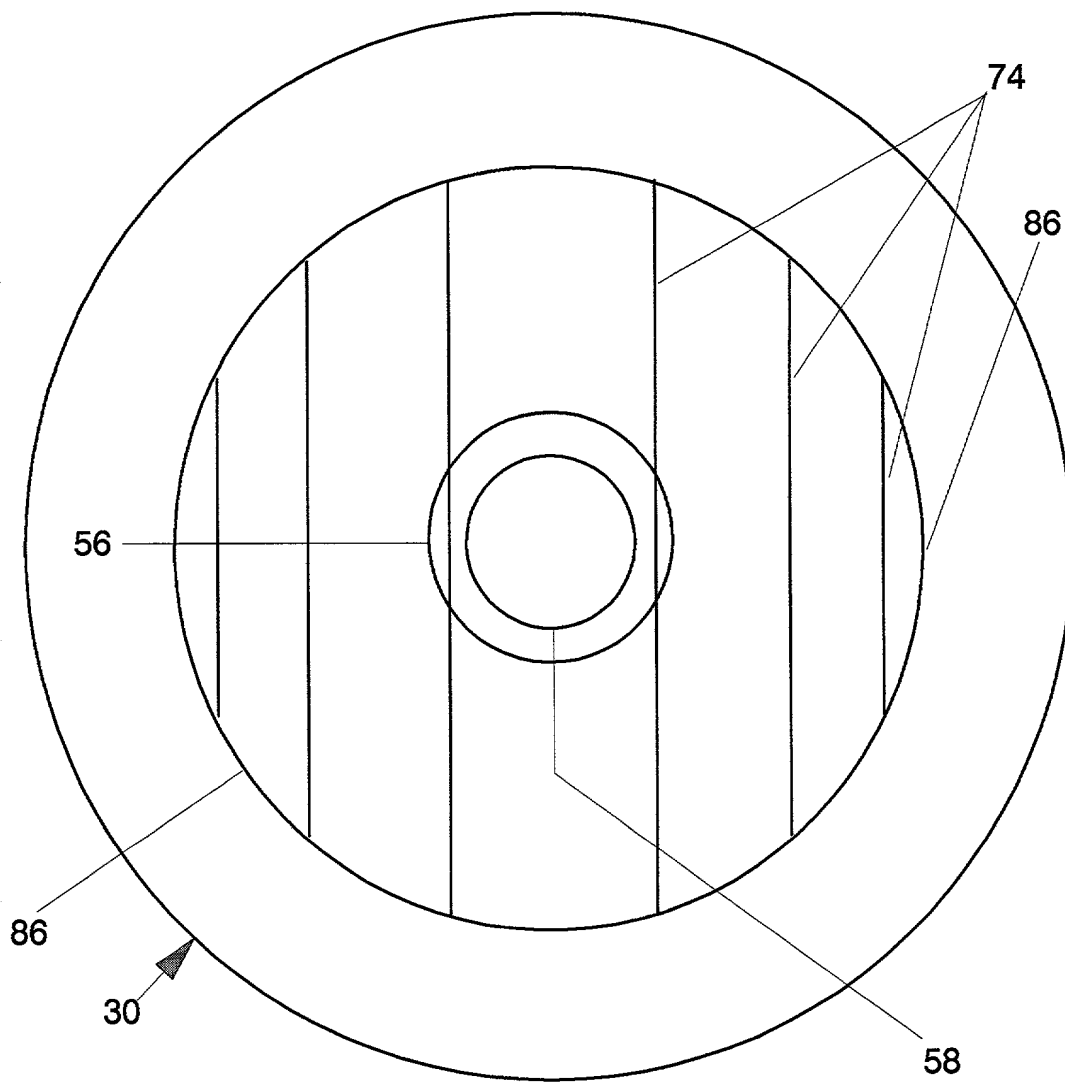


Fig. 5

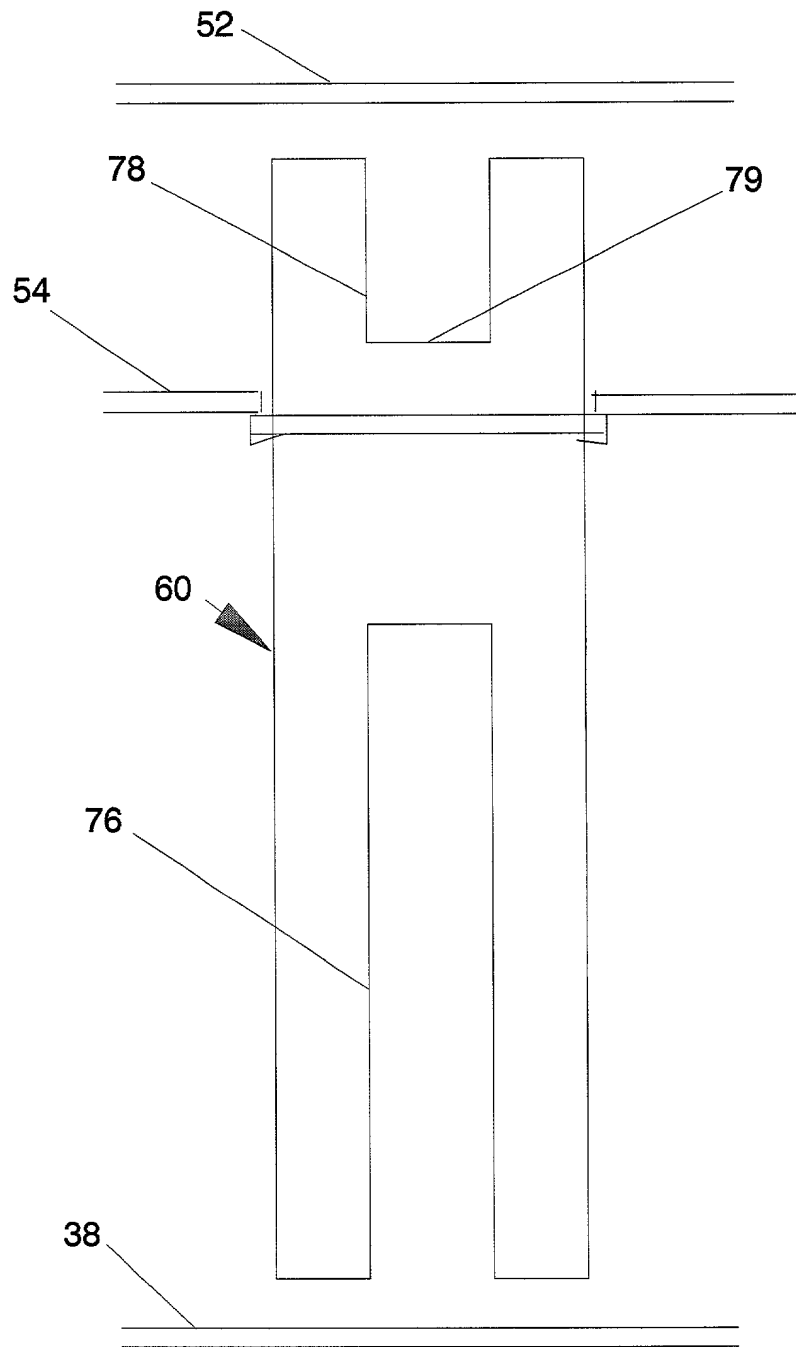


Fig. 6

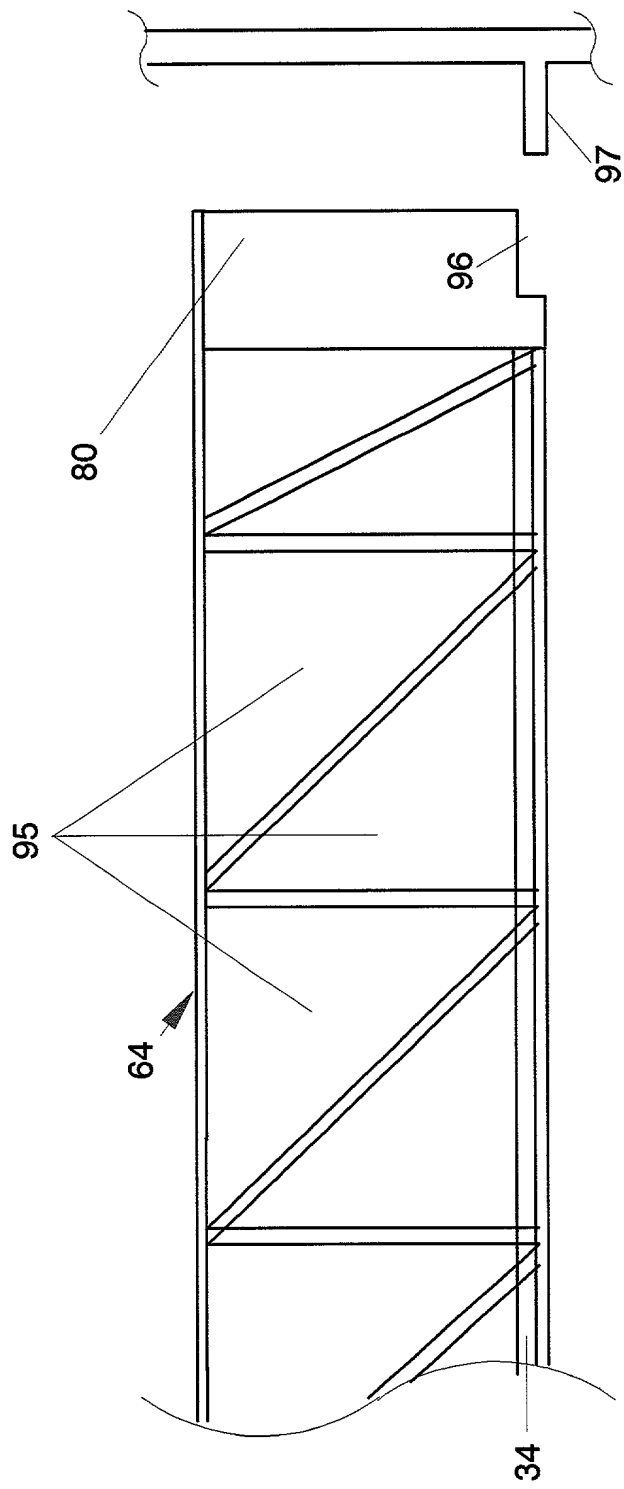


Fig. 7

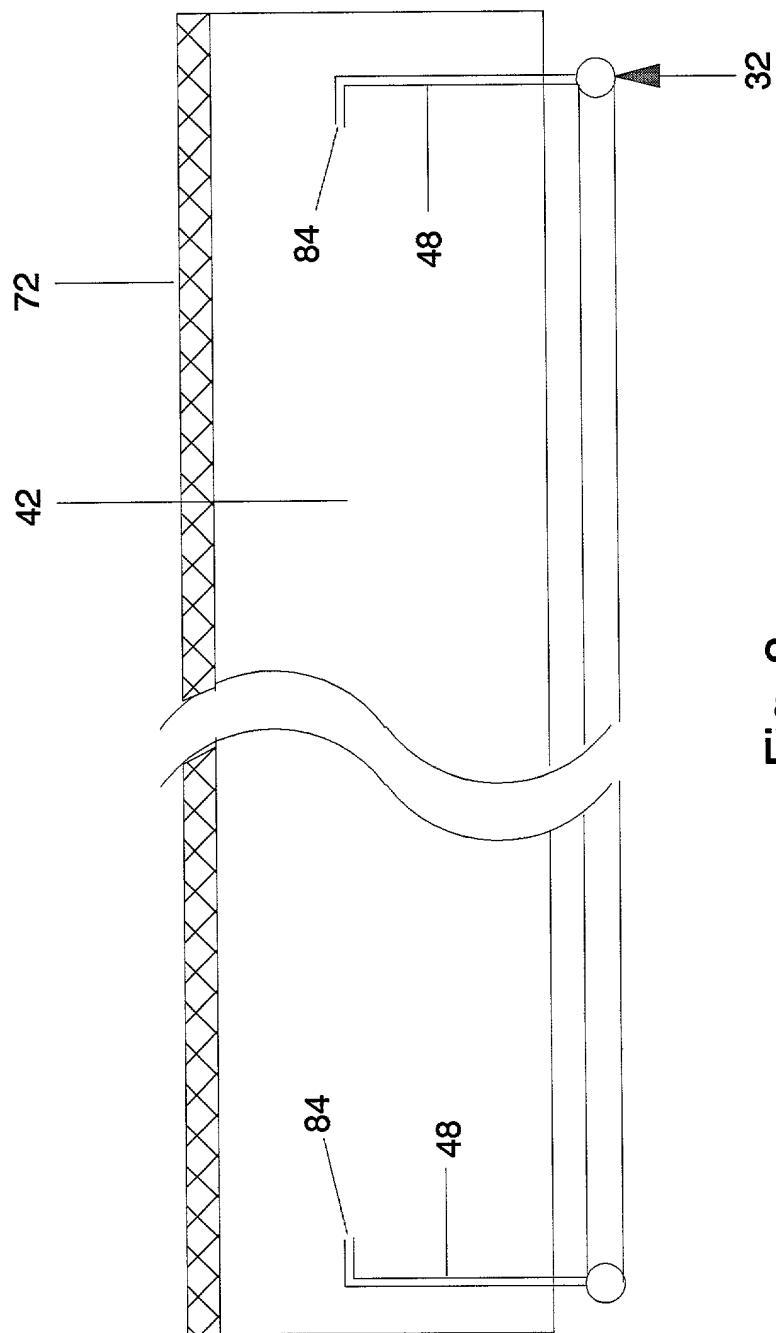


Fig. 8

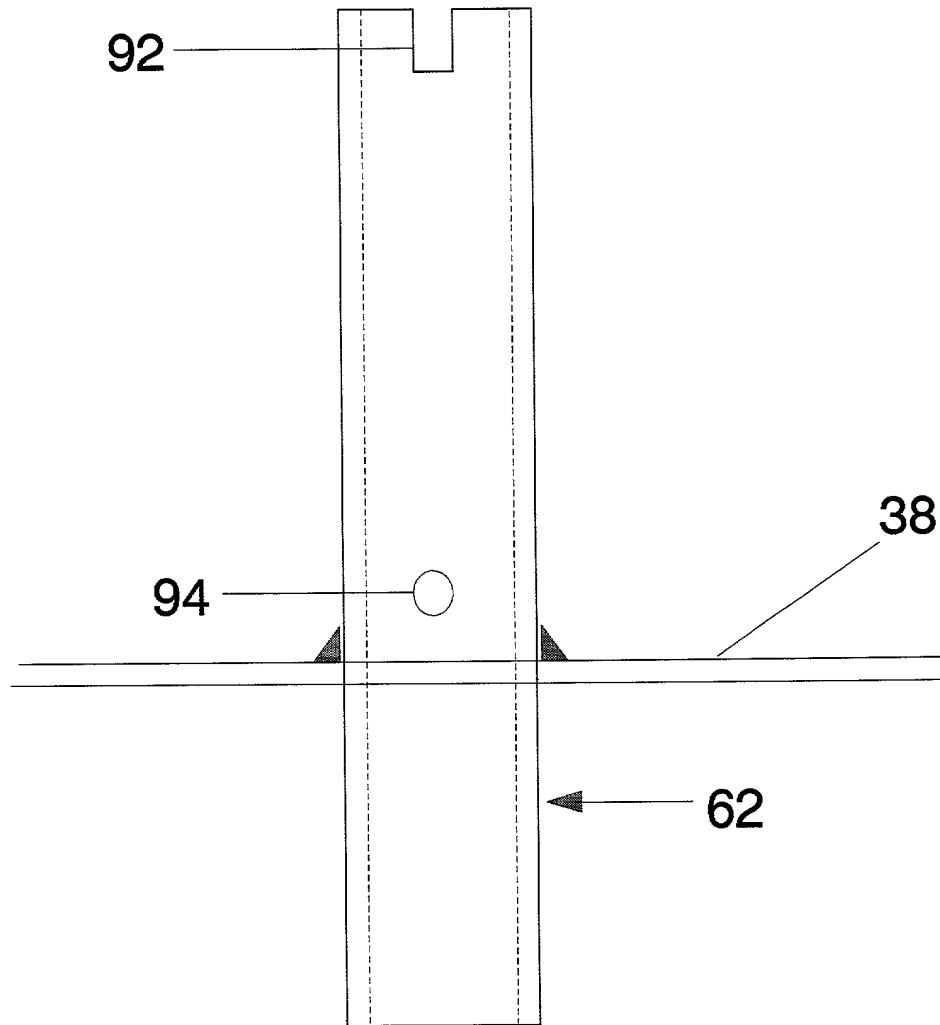


Fig. 9

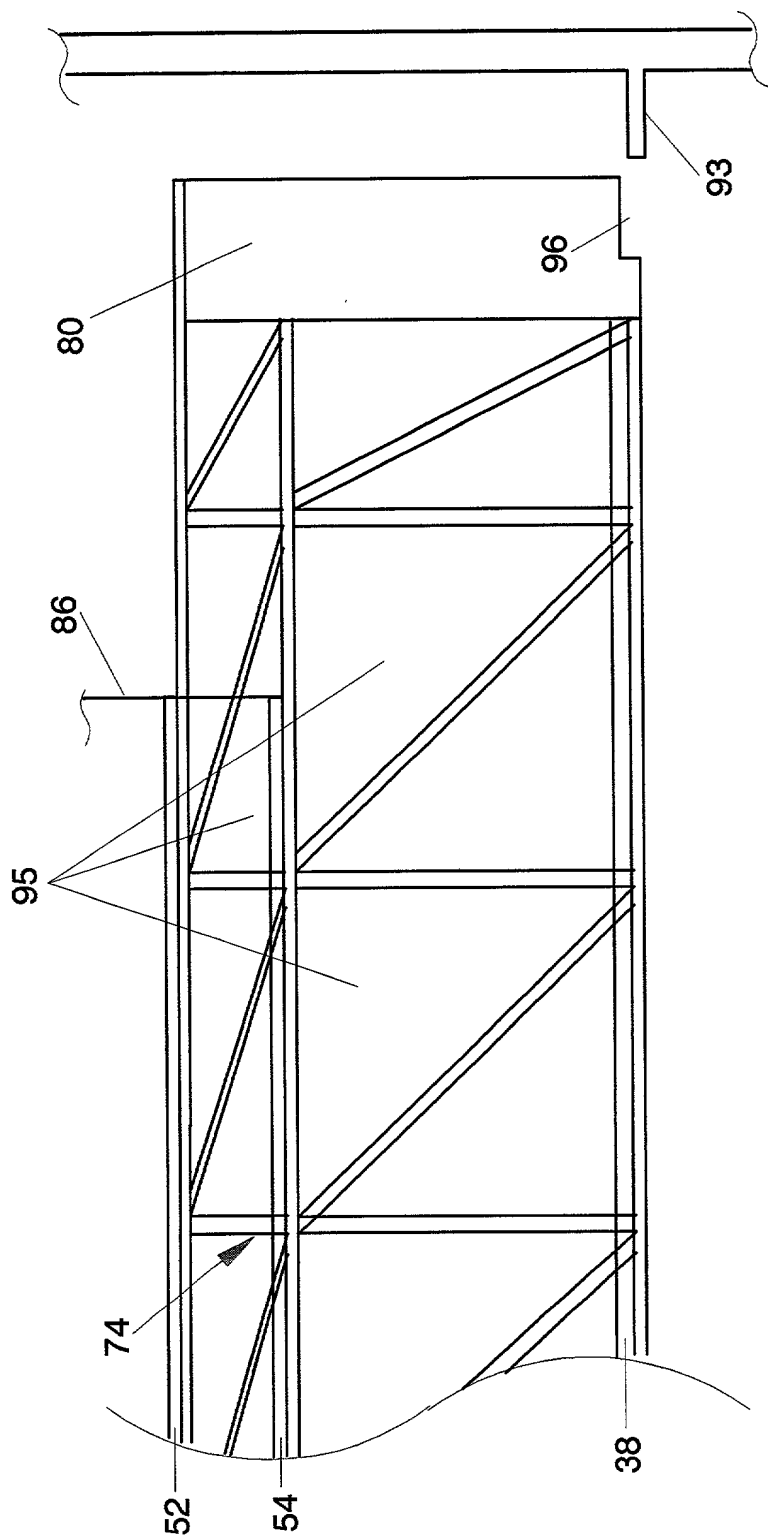


Fig. 10

FIG. 11 is a perspective view of the device in a first position, with the cover 34 in a closed position, and the device 50 in a first position, and the device 98 in a first position.

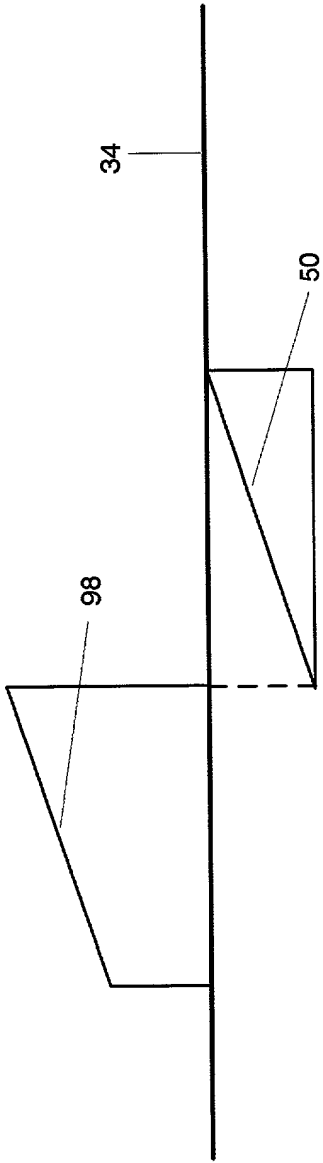


Fig. 11

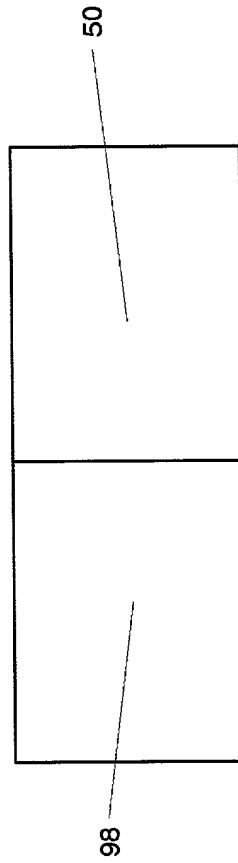


Fig. 12